

## *Quick Start Guide*

Levellogger Series



To begin using your Levellogger, download the newest version of Levellogger Software and User Guide by visiting: [www.solinst.com/Downloads/](http://www.solinst.com/Downloads/) or insert the software CD provided.

## Installing the Software

1. To activate the software install, click on the 'setup.exe' file located on the software CD.
2. The Software Installation Wizard will guide you through the remaining installation process.

## Installing the Hardware

1. Connect the communications device, either the Optical Reader or Interface Cable, to the computer.

**Notes:** USB connections require installation of a driver to the assigned device. See the USB Installation Guide for details.

## USB Installation Guide

**Notes:** 1. Levellogger Software comes pre loaded with necessary USB drivers.  
2. The following steps are based on the Windows® 7 operating system, if using another operating system, refer to the Levellogger User Guide.

1. Connect the USB device into the computer. This will begin the 'Found New Hardware Wizard'.
2. The 'Found New Hardware Wizard' will give the option to connect to Windows Update to search for software components, select "No, not at this time".
3. Two options are provided:
  - i. If you have the Levellogger Software CD, select "Install the software automatically".
  - ii. If you do not have the CD, select "Install from a list or specific location". In the next window select "Search for the best drivers in these locations" and "Include this location in the search".  
Select the browse button and choose this location:  
Program Files/Solinst/Levellogger 4\_0/USB Drivers

**Note:** During the USB Installation, a message may appear stating that the USB Serial Converter has not passed Windows Logo testing, select "Continue anyway".

4. Windows will confirm that the unit is now installed. Restart your computer. Repeat the above steps if your first install fails.

**If your device is plugged in and the Found New Hardware Wizard fails to start, then follow these steps:**

1. Open the Device Manager. Typically this is found through the path:  
Start > Control Panel > System > Hardware and Sound > Device Manager
2. Identify the Solinst device from the list. The device will be categorized under 'Other Devices' or 'Universal Serial Bus Controllers' (look for yellow warning icon).
3. Highlight the device in the list and right click. You will see an option to "Update the driver". This will start the 'Hardware Update Wizard'. Follow the steps for your operating system.
4. Once installed, the Com Port number will appear in Device Manager under 'Ports (Com & LPT)'.



PC Interface Cable




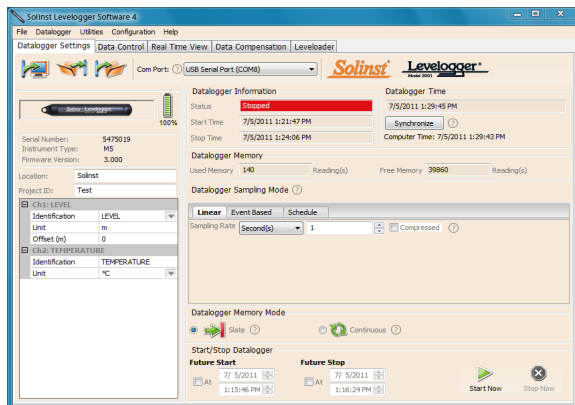
Optical Reader Connection

# Levellogger Series Quick Start Guide


## Programming the Levellogger

**Notes:** Ensure the Levellogger is operating with the latest firmware. Visit the Solinst website or software update feature for assistance.


1. Connect the Levellogger to the communications device and start the software.
2. Select the appropriate COM or USB port for the connected communications device from the centre drop-down menu.
3. Click the 'Retrieve Settings from Levellogger' icon. This will retrieve and display the current programmed settings for the connected Levellogger. 
4. You can now customize the Levellogger including your Project ID, Location, Sampling Mode and Rate, and Future Stop and Start times.



Datalogger Settings Window

**Note:** Clicking on the  embedded in the software will provide you with a short explanation of that feature, e.g. Com Port, Slate Mode, Time Synchronization, etc.


## Starting and Stopping the Levellogger

1. If desired, enter a Future Start and/or Future Stop Time.
2. When the 'Start' icon is selected, all settings are applied to the Levellogger and it will start logging at the specified time. 
3. To start logging immediately, do not fill in the Future Start field, and click the 'Start Now' icon.

**Note:** When the 'Start' icon is selected, a window will pop-up as an alert that the previous data will be erased.

4. To stop the Levellogger immediately, click the 'Stop Now' icon. 

### Tip

If a number of Levelloggers are to be programmed with identical inputs, clicking the 'Save Default Settings' icon will create a template. 



## Rainlogger Programming

The Rainfall Calibration Constant 'value' of the tipping bucket rain gauge used with the Rainlogger is required when programming the Rainlogger. Consult the Levellogger User Guide for more information on programming the Rainlogger.



## LTC Calibration

Before deploying your LTC Levellogger Junior, be sure to calibrate the instrument. To begin calibration, open the 'Conductivity Cal' tab and follow the steps provided. Consult the Levellogger User Guide for more information.

### Tip

The 'future start' and 'future stop' options are ideal for synchronizing the data collection of multiple Levelloggers.

## Downloading and Working with Data

1. Click the 'Data Control' tab to access the 'Data Control' window. This window is laid out in three sections: Levellogger settings, tabular data, and graphical data.
2. To download the data from a connected Levellogger, select the 'Download Data from Levellogger' icon. There are four options for downloading data. They are: All Data, Append Download, Partial Download and Recover Previous Log. The data will be presented in both tabular and graphical format.




**Note:** The default directory for downloaded and saved data is in the 'Data' folder:  
<C:\Program\Files\Solinst\Levellogger 4\_0\Data>.  
Data is saved as a \*.xle data file.

3. To save data, click the 'Save Data' icon and input desired name for the saved file.
4. To export the file for use in other software, click the 'Export' icon. The file can be exported to a \*.csv or \*.xml file.



### Note

To change the default directory for downloaded data, use the 'Configuration' menu at the top of the software window. Select 'Application Settings' and input or navigate to a different folder destination. Click 'OK'.

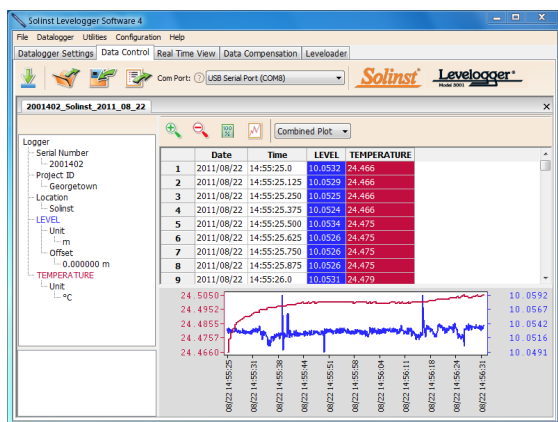


Data Control Window

### Tip

The \*.csv and \*.xml file formats are supported and can be imported by most spreadsheet and database programs.

The data graph can be exported to a \*.bmp file or a \*.wmf file by clicking File > Export > Graph.

## Real Time View

Real Time View provides on-screen measurement as data is being recorded by the connected datalogger. A view rate is set independently of the logging period of the Levellogger and does not interfere with internal logging taking place. To take a reading at any specific time, click  and that reading will be added to the displayed data. The data can be exported and saved.

## Compensate the Data

Click the 'Data Compensation' tab to open the Data Compensation window. In this window the 'Wizard' will guide you through Barometric Compensation, Manual Data Adjustments, Offsets, Altitude Correction, Unit Conversions, Density Adjustments, Conductivity Conversions, and Barometric Efficiency Compensations on your open data files. Multiple Levellogger files can be barometrically compensated at once, using one open Barologger file.

### Tip

'Manual Data Adjustment' allows you to use manual water level measurements to adjust your data to depth to water readings.

# Levellogger Series Quick Start Guide


## Levellogger Edge Field Measurement

### Levellogger Edge Ranges

Each model of Levellogger is rated for a specific submergence depth (Table 1). The choice of model largely depends on the accuracy of the water level required and the submergence depth. The selection, however, should be based on the maximum anticipated water level fluctuation.

Model	Submergence Depth	Accuracy
Barologger	Air only	$\pm 0.05$ kPa
F15, M5	16.4 ft, 5 m	$\pm 0.010$ ft, 0.3 cm
F30, M10	32.8 ft, 10 m	$\pm 0.016$ ft, 0.5 cm
F65, M20	65.6 ft, 20 m	$\pm 0.032$ ft, 1 cm
F100, M30	98.4 ft, 30 m	$\pm 0.064$ ft, 1.5 cm
F300, M100	328.1 ft, 100 m	$\pm 0.164$ ft, 5 cm

Table 1 - Levellogger Edge Range

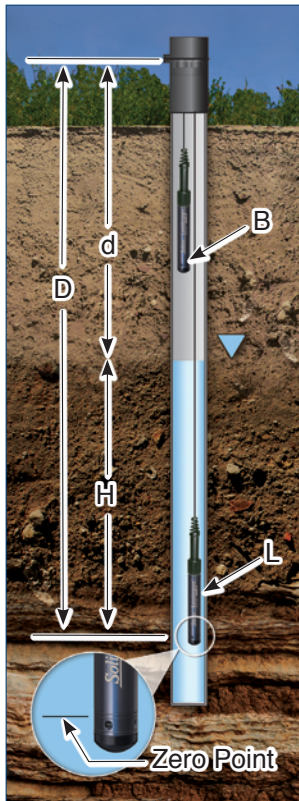

### Measurement Fundamentals

Levelloggers (L) measure the total pressure acting on a transducer at their zero point/sensor. The total pressure is caused by the column of water lying above the Levellogger pressure sensor AND the barometric (atmospheric) pressure acting on the water surface. To compensate for barometric pressure fluctuations and get true height of water column measurements (H), a Barologger (B) is required, i.e.:

$$\begin{aligned} &\text{Levellogger Reading (L)} \\ &\quad - \\ &\text{Barologger Reading (B)} \\ &\quad = \\ &\text{Height of Water Column (H)} \end{aligned}$$

### Verifying Readings

The best recommendation is to compare barometrically compensated Levellogger data (H) with a measured depth to water level value (d) (using a Water Level Meter). The deployment depth of the Levellogger (D), minus the manual depth to water measurement (d), should equal the compensated Levellogger reading, i.e.:

$$\begin{aligned} &\text{Deployment Depth (D)} \\ &\quad - \\ &\text{Depth to Water (d)} \\ &\quad = \\ &\text{Height of Water Column (H)} \end{aligned}$$

### Note

The Levellogger Edge can withstand over-pressurization of 2 times the intended range, e.g. a Model M10/F30 can accommodate a fluctuation of 20 meters or 60 feet and still record pressure. However, over-range accuracy is not guaranteed.



### Barologger Edge

A single Barologger can be used to compensate all Levelloggers on site, within a 20 mile/30 km radius and with every 1000 ft (300 m) change in elevation.

### Tip

To adjust all readings in your Levellogger file to depth to water below a well casing (d), record a manual water level measurement using a water level meter. This reading should correspond in date and time with an actual Levellogger recording. Use this as a reference datum in the Manual Data Adjustment option in the Levellogger Software Data Compensation Wizard.

## Levellogger Field Notes

### Before Deployment

Before deployment, make sure you do the following:

- Program your Levellogger, using Levellogger Software, with the correct project identification, memory mode, sampling regime, time, etc.

**Note: It is useful to synchronize the times of all Levelloggers and Barologgers being used for the same project.**

- Set a future start time, or start the Levellogger if deploying on a wireline/Kevlar rope (Levelloggers can be started after deployment if using a Direct Read Cable)
- Determine borehole depth to ensure Levellogger does not touch the bottom of the well (avoid submergence in sediment)
- Record the deployment depth of your Levellogger
- Use a Solinst Model 101 or 102 Water Level Meter to take a manual depth to water measurement that will be used to verify Levellogger readings
- Determine the minimum and maximum expected water levels, as Levelloggers must remain submerged for the entire monitoring period, and Barologgers must not be submerged

### Deployment


- Deploy your Levellogger and Barologger using a direct read cable for down-well communication, or use an inexpensive wireline or Kevlar cord.

**Note: For information on other types of installations, see the latest Levellogger User Guide.**

- Install the Barologger in a similar thermal environment as the Levellogger
- The Barologger should be suspended beyond the frost line and deep enough to avoid large temperature fluctuations
- Ensure the Barologger location is vented to atmosphere



**Wireline/Cord  
Deployment**

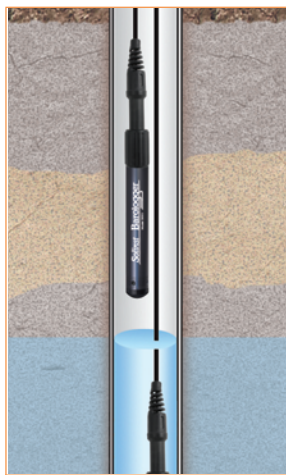

**Direct Read  
Deployment**

### Tip

*It is recommended to take a manual water level measurement before installing a Levellogger, shortly after installation, periodically during your monitoring interval, and at the end of your measurement period. Use these measurement to verify Levellogger readings, and for data adjustments later on. Ensure you take manual readings as close in time as possible to a scheduled Levellogger readings.*



### Well Caps

*The Model 3001 2" (or 4" with Adaptor) Well Cap Assembly provides a secure method of installing your Levellogger using wireline/Kevlar cord or Direct Read Cables.*

### After Deployment

After deployment, make sure you do the following:

- Take a manual depth to water measurement after the well has stabilized (approximately 10 minutes)
- Take another manual depth to water measurement just before removing the Levellogger from the well



# Levellogger Series Quick Start Guide

## In-field Communication

If you have installed your Levellogger using wireline/Kevlar cord, you can communicate with your Levellogger via an Optical Reader and Levellogger Software on a laptop PC.

If you have installed your Levellogger using a Direct Read Cable, you can communicate with your Levellogger via a PC Interface Cable and Levellogger Software on a laptop PC, or a Leveloader Gold, without removing the Levellogger from the well.



Optical Reader



PC Interface Cable



Leveloader Gold

## Frequently Asked Questions

### How can I protect my Levellogger from corrosive or marine environments?

The Levellogger Edge has a corrosion resistant Titanium-based coating. In harsher chemical environments, you can protect the Levellogger using a thin latex balloon filled with non-corrosive/non-toxic fluid (tap water). As pressure changes, the fluid encasing the loggers will transmit the pressure differential to the logger's pressure transducer, without exposing it to corrosive conditions.

### How do I install my Levellogger in a surface water application?

For installations within rivers, streams, wetlands, lakes and watershed or drainage basin monitoring, the shallow pressure range Levellogger Edge (M5/F15) or Levellogger Junior Edge (M5/F15) should be considered. For installation in streams or rivers, stilling wells can be constructed which shield the instrument from the water turbulence. Alternatively, Levelloggers can be lowered into a protective pipe or casing and then attached to a permanent fixture such as a bridge, pier or hand driven marker/rod.

### How do I protect my Levellogger from freezing?

To avoid icing/freezing and transducer damage, the easiest method is to lower the transducer to a point in the water column below the frost line or ice formation depth. In water bodies such as shallow streams, wetlands or ponds where icing/freezing may penetrate to the bottom, install the Levellogger in a vented stilling well imbedded into the bottom of the water body beyond the frost line.

If this is not possible, place the Levellogger inside two elongated silicon, rubber or latex balloons filled with a non-toxic, non-corrosive anti-freeze solution or saltwater solution. Place the balloons in a section of perforated, 1.25" (30 mm) ID pipe and install the logger in the monitored water. The antifreeze solution will protect the Levellogger from ice expansion at the pressure transducer, yet transmit any pressure and temperature fluctuations that occur.

# Troubleshooting Guide

## Levellogger Software:

1. You must have administrator privileges to install software on a computer.
2. Windows XP, Vista, and Windows 7 operating systems support Levellogger Software.

## Levellogger data has been accidentally erased:

If the Levellogger has been restarted and the old data has not been saved, select the download option "Recover Previous Log". This will download your previous data set.

## Communication Errors:

### "Port Cannot Open", "Check Com Port"

1. Reason: Software was started before USB device was connected to computer.  
Solution: Restart computer, connect USB device, start software.
2. Reason: Incorrect Com Port is selected in Com Port selection menu.  
Solution: Check the Com Port location for the installed device, by accessing the 'Device Manager' (through the Control Panel), and selecting the "Ports" section. This will state the Com Port the device is installed on.
3. Reason: Another device shares the same Com Port or is causing a communication conflict.  
Solution: Ensure that software for PDA or other devices, which automatically synchronize, are disabled. Ask your system administrator for assistance.
4. Reason: RS-232 Adaptor to USB converter is improperly installed.

**Note:** Not all converters are compatible with all makes and models of computers.

Solution: Reinstall supplied driver for converter device.

### "Communication Time-Out", "Communication Error"

1. Reason: Levellogger, Direct Read Cable, or communications device has failed.  
Solution: a) Narrow down the failure by using a different Levellogger, Direct Read Cable, or another communications device.  
b) Clean the optical "eyes" on the Levellogger and the cable, with a soft cloth.  
c) Check that the communication cable is connected to the same Com Port that is chosen in the upper middle of the Levellogger Software window.  
Check the Com Port settings. They should be as follows:
  - Bits per second: 9600
  - Data bits: 8
  - Parity: None
  - Stop bits: 1
  - Flow control: Noned) Try using a different computer, to see if this is the cause of the problem.  
e) If using a laptop (especially in conjunction with a Direct Read Cable) your Com Port may not be powered adequately to receive/transmit data. Try using a desktop computer to test this.  
f) If problem persists, contact Solinst.

**Note:** All Levelloggers should be deployed and stored with the installation cap or direct read cable attached. This prevents unnecessary battery drainage and protects the optical eyes.